


mackworth

FSG Portable Gantry

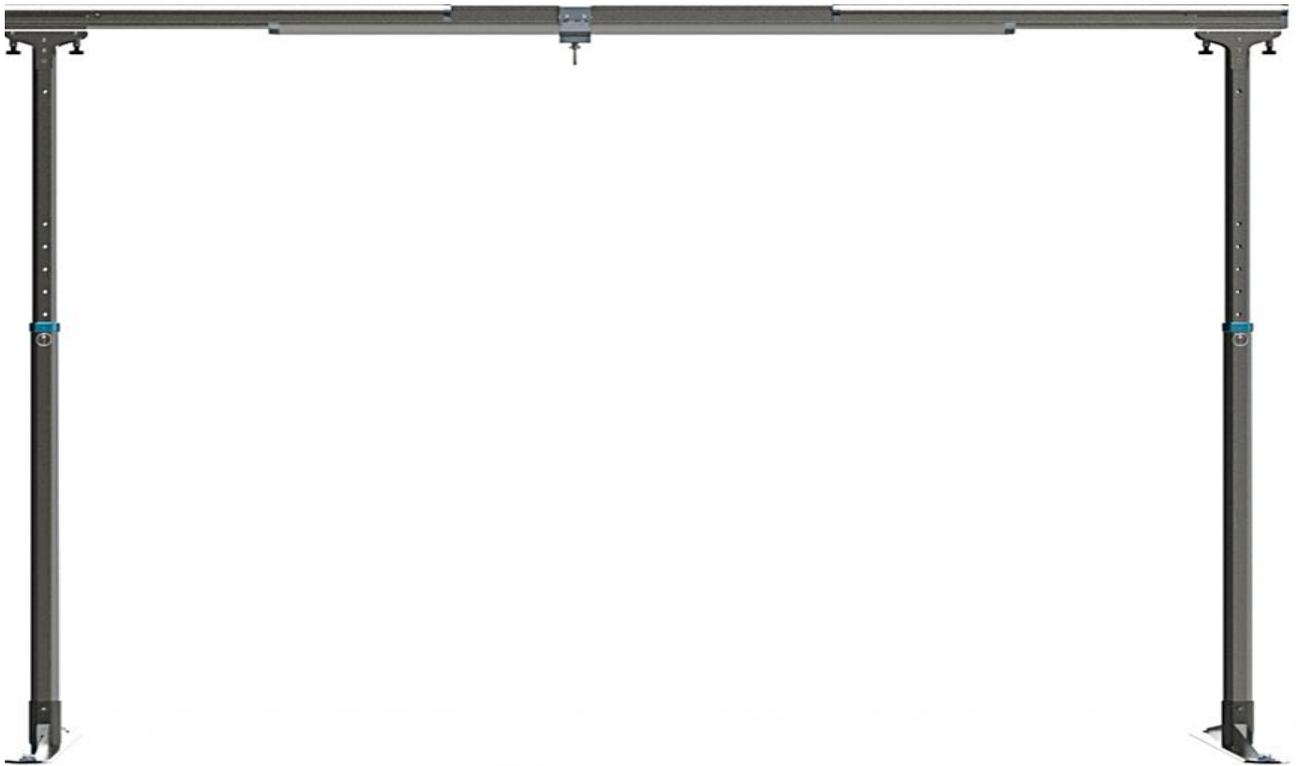

User Manual

1	Introduction	3
1.1	Intended Use	3
1.2	Manufacture	3
1.3	Symbols Used	4
1.4	Contraindications / Limitations	5
1.5	Safety Instructions and Warnings	5
2	Key Components	7
3	Gantry Adjustments.....	8
3.1	Adjust the Height	8
3.2	Adjust the Width.....	9
4	Technical Specification.....	10
5	Environmental Conditions	11
5.1	Operating Environment.....	11
5.1.1	Normal Operating Conditions	11
5.2	Storage Conditions.....	11
5.2.1	Shipping and Storage Conditions.....	11
6	Daily Checks.....	12
7	Cleaning	13
7.1	Gantry Cleaning	13
7.2	Disinfecting	13
8	Servicing.....	15
9	Troubleshooting.....	15
10	Disposal.....	16
11	Warranty	16
12	Service Record History	17

1 Introduction



Please read and understand this manual in its entirety before using your FSG Free-Standing Gantry. The information in this manual is important for the safety of anyone near the gantry and must be read and understood to help prevent injuries. It is also crucial to the proper operation and maintenance of the gantry.

This user manual should be kept safe for future reference. The contents of this manual are subject to change without prior written notice.

Should any questions arise from reviewing this manual, contact your local authorized representative.

If, during the use of this device, a serious incident occurs, please report it to the manufacturer and your national authority.

1.1 Intended Use

The portable free-standing gantry system is a great solution for situations where a permanent ceiling track cannot be installed. It is easy to set up and does not require any mounting on walls, ceilings, or the floor. The gantry is designed to work with a portable lift and sling, and together they form the portable free-standing gantry system. This system makes it possible to move individuals with mobility impairments with minimal strain or risk to the caregiver, while ensuring complete safety, dignity and comfort for the person being moved. It is important to note that the gantry is designed for internal use only and is not suitable for use in any other environment.

The gantry is designed to be operated by professional healthcare workers and home healthcare workers who may not have a specific range of skills in healthcare. Typical home-care users may include, but are not limited to, teachers, medics, paramedics, carers, family, and friends. Focusing on the dignity and well-being of the person being moved, the simple-to-use gantry maximizes the amount of care provided to the person.

You may need to seek specialist advice on how to assist some people with specific moving and handling needs. Sources of advice include, but are not limited to, professional bodies and organizations, occupational therapists, physiotherapists, manual handling advisers and ergonomists with experience in health and social care.

1.2 Manufacture

The product is manufactured at the address below:



Prism Medical UK

Unit 1, Tir Llwyd Industrial Estate,
St Asaph Avenue,
Kinmel Bay,
Conwy,
LL18 5JZ
Telephone number: 01924 840100

1.3 Symbols Used

The table below includes all symbols from BS EN ISO 15223-1:2021 that can be found in this manual and on the product, and what they represent. Refer to this table when you are unsure of what a symbol stands for.



			
Place of Manufacture	Country of Manufacture	Serial number	Catalogue number
			SWL
Caution – see instructions for use	Consult instructions for use.	UK Conformity Assessed	Safe Working Load
			
For internal use only	Packaging indicator – Keep dry	Do not use if package is damaged.	Packaging indicator – This way up
			
Fragile, handle with care	Please observe local laws on recycling.	Non-sterile	Atmospheric pressure limitation
			IP_{N1N2}
Temperature range	Humidity range	Class II Equipment	Degree of protection provided by enclosure. N1: Ingress of particles N2: Ingress of water
			
Type 'B' applied part	Type 'BF' applied part.	European Authorized Representative and Importer	Medical Device

Table 1-1

1.4 Contraindications / Limitations

There are no known "contraindications" associated with the usage of the gantry, provided it is used as per the manufacturer's recommendations and guidelines. However, it is recommended that a client-specific assessment be completed by a trained and knowledgeable health care professional to determine the method of transfer and use.

The manufacturer does not recommend a required number of operators for the use of the products. This information and recommendation can only be provided after a thorough, personalized, case-specific assessment, as many factors can influence these decisions.

Limitations of the Gantry include:

- The gantry should only be operated by competent and trained people.
- The gantry should only be used with patients weighing under the safe working load of the gantry.
- Between the gantry, portable lift and sling, the lowest safe working load of the components should not be exceeded.
- The gantry is only to be used with the portable lift that is installed on it. The gantry must only be relocated by an authorized person.
- The gantry is only compatible with the allocated portable lift and slings found within this manual.
- The gantry is designed for human transfer only. There is no other application for this product.
- The operator of the gantry must always pay attention to the well-being of the patient. Patients should not be left unsupervised during the operation.

1.5 Safety Instructions and Warnings

Ensure to read and understand all the statements below, for the safety of the caregivers and users, along with warranty requirements. Failure to follow warnings in this manual may result in injury to the operator and/or client and/or damage to the gantry or related components.

- If you are unsure of the correct use of this product, please contact the manufacturer or a professional for further information or training.
- The gantry is intended to be installed on a flat and level surface before use.
- The gantry must be installed only by people authorized by the manufacturer or who have the right to install and commission the gantry safely for use.
- The gantry and associated portable lift and accessories are not toys. Do not use it for unsafe practices. Do not allow children to play with the product or any of its components. The gantry should not be used for any practice except its intended use.
- In facilities where more than one operator will be responsible for using the gantry, it is important that all such members be trained on the product before use. A training program should be established by the facility to acquaint new operators with this equipment.
- Your guarantee is void if people unauthorized by the manufacturer perform work on the gantry.
- To maintain optimum function, the product should be inspected and maintained regularly. See section 'Daily checks, Servicing and Cleaning' within this user manual.
- The gantry and its associated portable lift are intended only for the transfer of a person. The manufacturer will not be responsible for any damage caused by the misuse, neglect, or purposeful destruction of the equipment and/or its associated components.
- Any accessories used with the product should be checked before each use to ensure that they are in good working order. Check signs of wear and ensure that all labels are legible. Report any unusual wear to your local authorized dealer.

- Ensure that a clear space is maintained around the gantry. Before using the gantry, always check for and remove any obstacles.
- Never leave a user unattended in the gantry.
- If additional accessories have been supplied with the gantry, refer to the instructions included with those items.
- Under no circumstances should the gantry, associated portable lift, sling, or entire system be put under the control of a person who has not been properly trained in the use and care of this equipment. Failure to adhere to this warning may result in serious injury to the operator and/or the individual being lifted and transferred.
- Unauthorized modifications to this product may affect its safety. The manufacturer will not be held responsible for any accident, incident or deficiencies of performance that occur because of any unauthorized modification to its products. Your guarantee is void if any modifications are made that are not authorized by the manufacturer.
- The gantry and associated accessories, portable lift and sling(s) are intended only for the transfer of a person. We will not be responsible for any damage caused by the misuse, neglect, or purposeful destruction of the gantry and/or its associated components.
- The installation of the gantry and its associated parts is certified to have a maximum load of 200 kg (440 lb.). Do not exceed the maximum rated load of any of the components.
- Your gantry is for aiding and transferring a person. Do not use it, or allow it to be used, for any other purpose.
- In areas where children are prone to be present, be vigilant when using the gantry.
- To reduce the risk of unintended use, when the gantry is not in use, remove the sling(s) from the portable lift to prevent entrapment or strangulation should the device be tampered with.
- Between the gantry, portable lift, and sling, the lowest maximum load shall always be used.
- A risk assessment must be performed before using any other manufactured sling, carry bar or portable lift to ensure 'safe' use can be established.
- Risk of collision: The person using the portable lift on the gantry should make sure that when raising, lowering, or moving the lift along the gantry that no people or objects will obstruct, be injured or damaged by the movement.
- Serious Injury: If, during the use of this device or because of its use, a serious incident has occurred, please report it to the manufacturer and your national authority.



You may need to seek specialist advice on how to assist some people with specific moving and handling needs. Sources of advice include, but are not limited to, professional bodies and organizations, occupational therapists, physiotherapists, manual handling advisers and ergonomists with experience in health and social care.

2 Key Components

Please see below to familiarize yourself with the components of the gantry. The images below show the contents of the gantry. If you have not received all the components, contact your local dealer immediately – contact details are provided on the last page of this manual.

Item	Description
1	Adjustable Track
2	Info Label
3	Support Post
4	Foot
5	User Manual

Table 2-1

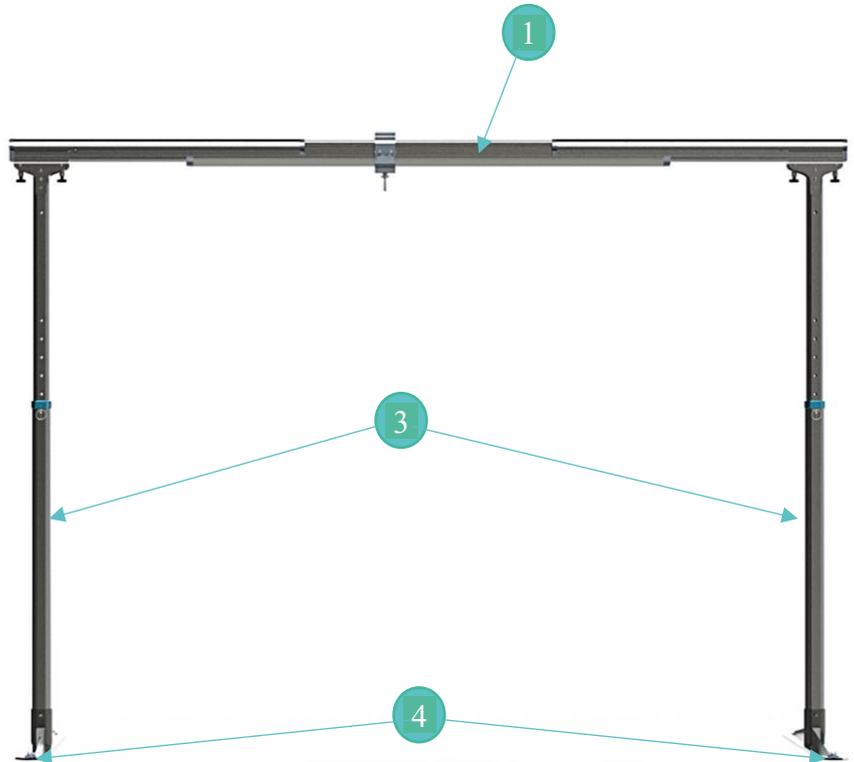
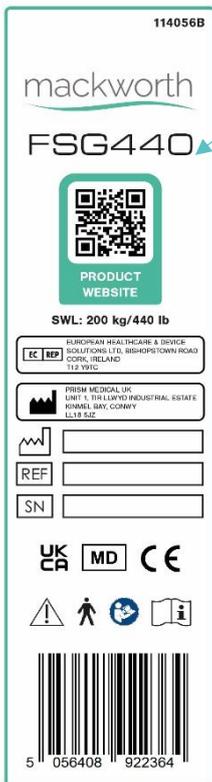


Figure 2-1

(Located on both gantry support posts)

*Disclaimer: The label shown is for illustrative purposes only and may not represent the actual label affixed to the product. Refer to the product itself for accurate and current labelling information.

3 Gantry Adjustments

If you need to adjust the height and width of the gantry, it's important to do so safely. We recommend that two people work together to carry out these adjustments. To ensure a safe and effective adjustment, please follow the guidelines below:

3.1 Adjust the Height

1. To adjust the height of the gantry, first remove the safety and lynch pins found on both support posts, as per Fig. 3.1-1



Figure 3.1-1

2. Press the latch found on the support post and raise the track vertically until the desired height has been reached. It is recommended that this be done on both posts at the same time. See Fig. 3.1-2



Figure 3.1-2

3. Once the desired height has been reached, release the latch, and ensure it locates into the nearest hole found on the moving post. Make sure this is done on both support posts and that the posts are set to the same height. See Fig. 3.1-3 and then re-insert the safety and lynch pins to both support post.



Figure 3.1-3


4. If required, adjust the self-leveling screws to improve stability, which are located on the foot as shown in Fig. 3.1-4.




Figure 3.1-4

3.2 Adjust the Width.

1. To adjust the width of the gantry, first lift one of the support legs vertically up off the floor.
2. Then adjust the support leg by pushing or pulling it inwards or outwards according to your requirements. If necessary, repeat the process for the other leg. Refer to Fig. 3.2-1 & Fig. 3.2-2 and ensure that you have the assistance of two people to support both legs and, at the same time, to ensure a safe adjustment.
3. Once the gantry is at the desired width, place the support leg back onto the floor.
4. If needed, you can also adjust the self-levelling screws located on the foot to improve stability as shown above in Fig. 3.1-4.

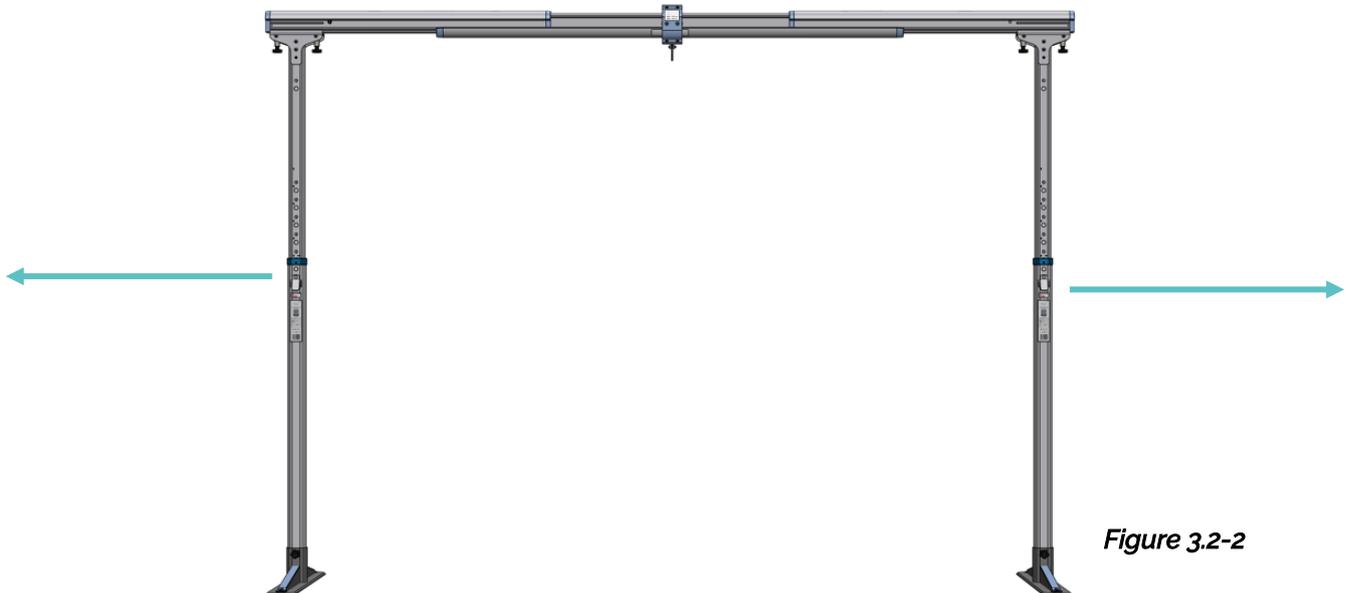

4 Technical Specification

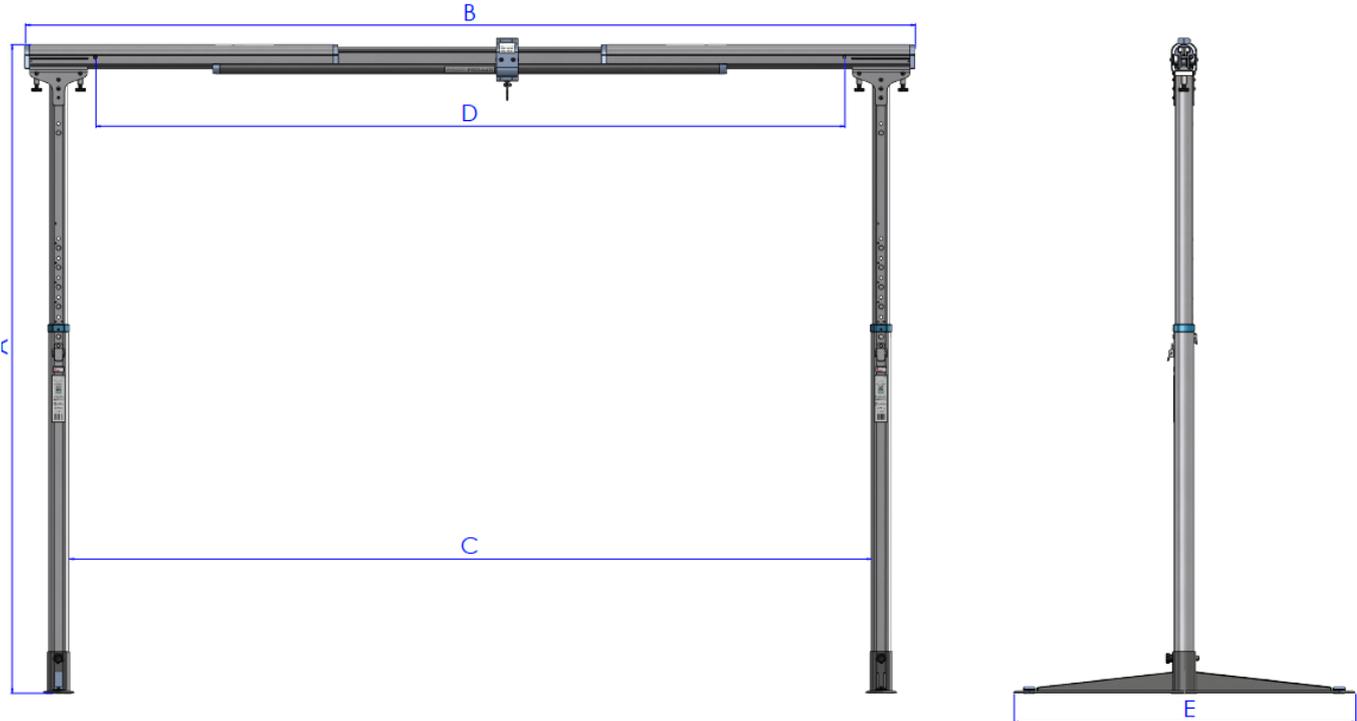

Gantry Dimensions		
A – Min-Max Height	84.3" – 98.7"	
B – Min-Max Width	96.3" – 13.3"	
C – Min-Max Internal Clearance	82.8" – 120.2"	
D – Min-Max Horizontal Travel	74.8" – 112.2"	
E – Foot Length	51.2"	
General		
User Maximum Weight	440lb	
Product Weight	< 50lbs	
Expected Lifetime	10 yrs	
Construction Type	Aluminum	
Packaging Specification		
Track Box Weight	< 45lbs	
Leg and Foot Box Weight (each)	< 30lbs	
Track Box Dimensions (L x W x H)	95.4" x 11.4" x 4.7"	
Leg and Foot Box Dimensions (L x W x H)	64.8" x 11.3" x 9"	
Applied Standards		
EN ISO 15223-1:2016	IEC 62366-1:2015	
EN 1041:2008+A1:2013	BS EN ISO 14971:2019	
BS ISO 20417	BS EN ISO 10535:2006	
Certifications & Accreditations		

5 Environmental Conditions

The sections below will give detailed information regarding the environmental conditions the product should maintain throughout its life cycle. Failure to adhere to these conditions may negatively impact the function of the product. If you are unsure of any environmental conditions, always seek advice.

5.1 Operating Environment

The gantry is intended to be used in dry environments. The gantry is intended for internal use only.

The gantry is intended to be used within a professional healthcare facility or home healthcare environment. The gantry is not suitable for any other environment.

The gantry is not intended to be used in environments where there are rapid changes in the environmental temperature and humidity.

The gantry suffers little from any effects of lint, dust, and light.

- Lint – Due to the nature of the gantry being installed close to the ceiling, very little lint would be likely to gain access into the gantry's workings. The gantry is recommended as per the User Guide to be wiped clean during every gantry inspection.
- Dust – Due to the nature of the gantry being installed close to the ceiling, very little dust is likely to gain access into the gantry's workings.
- Light – The user adjustments have been designed to be easily recognizable within the specification of the gantry's ambient luminescent range of 50 – 500 lux. Within this range, there are no effects on its operation. Additionally, the gantry is designed for indoor use only; if required, the user may wish to switch on room lighting.

5.1.1 Normal Operating Conditions

+5°C to +40°C (41°F to 104°F) at a relative humidity between 15% to 90% RH, non-condensing but not requiring water vapor pressure greater than 50hPa and atmospheric pressure between 795hPa to 1060hPa.

5.2 Storage Conditions

The gantry is intended for internal storage within normal environmental conditions. The gantry is intended to be stored in a dry room.

It is not intended to be stored in environments where there are rapid changes in the environmental temperature.

When storing the gantry, ensure that the product has been cleaned and dried. For further information, refer to the 'cleaning' section instructions.

5.2.1 Shipping and Storage Conditions

-25°C to +5°C (-13°F to 41°F) with any humidity level.

+5°C to +35°C (41°F to 95°F) at a relative humidity up to 90%.

+35°C to 70°C non-condensing at a water vapor pressure up to 50hPa.

6 Daily Checks

Inspection is to be completed prior to each use by the user of the gantry.



Should any of the components in the table below fail the inspection, DO NOT use the gantry. Contact your local authorized dealer for service – contact details are on the last page of this manual.

Ensure all component inspections in the table below are completed before each use of the gantry.

Check List before Use:

Component	Service/Inspection required
Generic	Visual inspection of the exterior of the gantry. Significant damage that may affect the function of the gantry, along with a clear safety hazard, is unacceptable.
	Check the labelling on the gantry to ensure they are all still legible, this includes the serial number and other important markings. If labels are not legible, then contact your local authorized dealer immediately.
	Check that the gantry is level and the feet are located on a stable level surface.
	Check that the safety pins are installed in both support posts.
	Check that all fixing points are tight, and no parts are broken or bent. If they are not tight or you have concerns, then contact your local authorized dealer immediately.
Trolley/Wheels	Ensure the wheels are traversing smoothly in the gantry before traversing a patient along the system. Listen for any unusual noises.
	Ensure that the locking device on the QRS is closed when attached to the trolley.

7 Cleaning



To reduce the risk of cross-contamination, it is recommended to clean the gantry and accessories before use by a different person.

Please follow the recommended cleaning guidelines below for cleaning and disinfecting the gantry.

7.1 Gantry Cleaning

For cleaning, the gantry can be cleaned using a damp cloth, soap/water, and antibacterial spray. Do not use a steam cleaner as this could damage the gantry as well as the label integrity. Do not use industrial bleaches, abrasive cleaners, or organic solvents.

All cleaning solutions must be thoroughly rinsed off the product at the end of the cleaning process, and the product must be dried using a dry cloth/towel. Always ensure the product is dry before use.

7.2 Disinfecting

Should the gantry require a more thorough cleaning, the use of the Actichlor™ disinfectant product (which is widely available in tablet form and used throughout the healthcare industry) is recommended.



Follow the manufacturer's safety instructions for the use of this cleaning product before use to ensure safe use for the operator and the user.

Ensure the cloth is damp before the cleaning process.

The application is through a clean, damp cloth, which is used to wipe the product down. Use the following dilutions to ensure effective cleaning:

- Actichlor™ dissolvable chlorine tablets provide a concentration of 1000 ppm of available chlorine (0.1%) per 1 tablet.
- 1 tablet (1.7g formed tablet (x1)) will create a virucidal solution, diluted in 1 litre of water to provide effective means to clean a "dirty" product. This is also ideal for use after an outbreak of the Norovirus/winter vomiting and can be used as a precaution against C.Diff. It is effective against viruses, bacteria, spores, yeasts, and molds.
- A minimum of 5 minutes contact time with the outer components is recommended to prevent virucidal infections, whilst maintaining the integrity of the product. The product can withstand a longer contact period, however, a minimum of 5 minutes is required to provide an effective cleaning regime.
- Blood spills should be dealt with by an increased concentration of the solution – please refer to the instructions on the manufacturer's product labelling.

Dilution chart					
Product used as	Product condition	Concentration (ppm)	Dilution qty* (l)	Tablets per 1l (0.26gal)	Contact time (minutes)
Bactericidal	Clean	200	5 (1.32 gal)	1	1
	Dirty	1000	1 (0.26 gal)	1	5
Yeasticidal	Clean	200	5 (1.32 gal)	1	1
	Dirty	1000	1 (0.26 gal)	1	5
Fungicidal	Clean	2000	1 (0.26 gal)	2	15
	Dirty	5000	1 (0.26 gal)	5	15
Mycobactericidal	Clean	1000	1 (0.26 gal)	1	15
	Dirty	5000	1 (0.26 gal)	5	15
Virucidal	Clean	500	2 (0.53 gal)	1	5
	Dirty	1000	1 (0.26 gal)	1	5
Sporicidal (C. Diff)	Clean	1000	1 (0.26 gal)	1	10
	-	-	-	-	-
Sporicidal	Clean	5000	1 (0.26 gal)	5	10
	-	-	-	-	-

- Dilution is made with water. DO NOT dilute within any other medium.
- When diluted in water, one tablet gives 1000 ppm of available chlorine.
- The concentration of the solution depends upon whether the object being cleaned is noticeably dirty (indicated in the table by "Product condition").

Table 8.2-1

Handling and storage safety precautions when using this cleaning agent:		
Advice on Safe Handling	Hygiene Measures	Conditions for Safe Storage
<p>Avoid contact with skin and eyes.</p> <p>Do not breathe dust, fumes, gas, mist, vapor, or spray.</p> <p>Use only with adequate ventilation.</p> <p>Wash your hands thoroughly after handling.</p> <p>Mixing this product with acid or ammonia releases chlorine gas.</p>	<p>Handle in accordance with good industrial hygiene and safety practice.</p> <p>Remove and wash contaminated clothing before re-use.</p> <p>Wash face, hands, and any exposed skin thoroughly after handling.</p>	<p>Keep out of reach of children.</p> <p>Keep the container tightly closed.</p> <p>Store in suitable, labelled containers.</p> <p>Storage temperature: 0-25°C (32-77°F).</p>
Individual Protective Measures	Dissolve	
Hand protection: Gloves	Dissolve in cold water – With no agitation, 1 tablet will take approximately 10 minutes to fully dissolve in the water used.	
<p>The information above has been extracted from the Actichlor™ MSDS (Manufacturers Safety Data Sheet). For a full review of the data, please follow the link below:</p> <p>http://www.nhsggc.org.uk/media/236215/msds-actichlor-plus.pdf</p>		

Table 7.2-2

8 Servicing

Regular service on the gantry will help prevent breakdowns and reduce repair costs. It will also improve the quality of the product for the end users.



To reduce the risk of injury, no service is to be carried out on the gantry while in use. Service must be completed by an authorized service engineer only. Do not try to service the product yourself; this will void your warranty.

To ensure the safety and continued good function of your gantry, it is recommended to have an approved service engineer perform a routine service every 6 months. This will ensure that the product meets the required standards. It is important to document the service history of the product in the service log found at the back of this user manual after each service.

When the product is serviced, the service checklist must be completed.
Service Manual Document Number: 995548.

For information about spare parts, refer to the spare parts manual.
Spare Parts Manual Document Number: 992548.

Contact your local authorized dealer if you:

- Need more information.
- If you have any questions about the use or service of your product.
- Notice any change in the performance.
- If you want to report an unexpected occurrence.
- If you want to arrange a service.
- Need to find the necessary information for replacement parts and components.

The expected product lifetime is **10 years**. This is dependent on usage and compliance with maintenance and servicing. Regular service on the product will increase the expected lifetime.

9 Troubleshooting

Should a problem arise with the use of the gantry, review the table below. Find the fault and complete the recommended solution. If the fault is not listed below or the solution does not correct the problem, contact your local authorized dealer at once – contact details are provided on the last page of this manual.

Fault	Action
The trolley does not traverse	<ul style="list-style-type: none"> • Check that the track profile is clean and free from any obstructions. • Check the wheels are free and regular service has been undertaken. • Check that the telescopic track profiles are all aligned.
Portable lift transverse without assistants	<ul style="list-style-type: none"> • Check that the gantry is located on a level surface. • Check that the installation of the gantry has been carried out correctly. • Check that the traversing track is level.
The gantry is unstable.	<ul style="list-style-type: none"> • Check that the gantry is located on a level surface. • Ensure all foot contact points are in contact with the floor. • Ensure that the track attachment star handle bolt is all secure.

Table 9-1

10 Disposal

With efforts to improve the environment and reduce waste, where possible, our products have been manufactured with recyclable materials. Below are our guidelines on recyclable materials and being environmentally friendly.

The gantry should be disposed of by an approved service engineer at the end of its life cycle.

Please see the local laws on recycling and respect the current laws for disposal within the community where the product is being used. If there is any uncertainty about the guidelines below, contact your local authorities to decide the proper method of disposal of potentially biohazardous parts and accessories.

Fully recyclable:	Considerations when Recycling:
Aluminum structure (Track, support posts, feet)	Plastic parts (end caps, foot covers)
Steel trolley	
Initial packaging of the device (cardboard)	
Metallic fixing – screws etc.	

Table 10-1



The product may be contaminated and must be disinfected before recycling or disposal. See the section on 'Cleaning' for further details.

11 Warranty

It is impossible for all the risks to be eliminated from the use of this product, but to reduce risk and improve safe and proper use, the user should always read and understand the user manual before use. Product failure may occur due to a lack of maintenance and care, misuse, unauthorized and improper servicing or alterations, improper storage, environmental use, or through normal wear and tear. These factors are all beyond the control of the manufacturer. These risks are taken on by the users.

The gantry comes with a 1-year warranty covering all manufacturing defects. Refer to your terms and conditions for more detailed information. The warranty is valid if the product has been maintained in its intended use and the user manual instructions have been followed. The warranty will not extend to the use of the product when used contrary to the user manual. This guarantee does not affect or in any way limit your statutory rights.

1. The liability of the manufacturer under the terms of this guarantee shall be limited to the replacement of the defective part(s) to the sales distributor, dealer, agent, person, or entity which purchased the equipment from the manufacturer. In no event shall the manufacturer incur liability for any consequential or unforeseen losses.
2. This equipment guarantee shall be void if an authorized service engineer does not service the equipment, in accordance with the manufacturer's recommendations, or if any unauthorized people carry out work on the equipment.
3. This guarantee does not apply to failure attributable to normal wear and tear, damage by natural forces, user neglect or misuse or deliberate destruction.
4. Do not try to service the product yourself, or the warranty is void.

12 Service Record History

Complete this section after each service, repair, inspection and/or maintenance.

Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	

Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	

Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	

Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	

Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	

Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	

Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	
Date:	Time:
Service Type: Service Inspection <input type="checkbox"/> Repair <input type="checkbox"/> Other <input type="checkbox"/>	
Completed By: (Printed name) (Signature)	
Company:	
Remarks & Actions Taken:	
Product Left in A Safe & Usable Condition: Yes <input type="checkbox"/> No <input type="checkbox"/> (if no, explain in actions above)	

Dealer/service contact details:

Contact details:

Mackworth USA
54 West Industrial Drive
O'Fallon, MO 63366 USA
314-889-1000
www.mackworthusa.com

Disclaimer

While every effort has been made to ensure the accuracy of information contained in this manual, no liability can be accepted by Mackworth for any errors or omissions. Mackworth operates a policy of continuous improvement. Specifications and other data are subject to change without notice.

